

TransTech Systems, Inc.



SDG  200

Quick Start Guide

Scan for additional manuals & guides
or visit www.transtechsys.com/products/resources



Table of Contents

Contents	3
Charging Batteries	4
Starting the Software	5
GPS Setup	6
Control Menu	7
Unit Settings	8
Material Details	9
Edit Material	10
Project Details	11
Soil Reading	12
Data Management	14
Upload Material	15
Replacement Parts	18
Warranty	19

Contents

**Fold open
compartment
contents**

**Charger
AC Cord
DC Cord
Handle**



**Slot for
SDG 200 and
Standardization
Plate**

Case



SDG200



**Standardization
Plate**



DC Cord



AC Cord



Handle



Charger

Charging Batteries



1. Turn the SDG 200 unit OFF.
2. Connect the charger to the charger connector located on the back of the SDG 200.
3. Plug the charger into a standard AC outlet.
4. The red indicator lamp will turn green to indicate that the batteries are charged. (approx. 4hrs)
5. Unplug the charger from the power source before disconnecting the charger from the SDG 200.

Battery Care Tips

- Whenever uncertain about the battery charge level or condition, recharge it
- The battery will self-discharge and should NOT be left uncharged for more than 30 days
- An occasional complete discharge followed by a full recharge is recommended
- **NEVER** drop the battery as this can damage the internals
- **DO NOT** store in freezer or expose to extreme heat
- Battery should be fully charged before use

Starting the Software

Pressing the ON button will power on the SDG 200. After a few seconds the TransTech splash screen will appear followed by the Main Menu screen. The Main Menu screen will display five options, **Start SDG200**, **GPS Control**, **Calculator**, **Contact TransTech** and **Update Software**.



Unit Settings

From the **Main Menu**, press **GPS CONTROL**. GPS status can be toggled ON or OFF. When enabled the satellite dish icon on the status bar at the bottom of the display turns from red to green.

GPS formatting can also be toggled from the **Universal Transverse Mercator (UTM)** grid to **Latitude/Longitude (LAT-LON)**. Initially the display will read Sats 0 for both formats until connections have been made. The below example shows a connection to five satellites (Sats 5). GPS locations will appear on the bottom left corner of the soil reading screen and will store with each reading when enabled. Press **Main Menu** to return to the Main Menu.



GPS Enabled



GPS Disabled


Data Logging

From the **Main Menu**, press **Start SDG 200** to enter the **Control Menu**. From this menu, you will select units as well as material and project information.



Unit Settings

From the **Control Menu**, press **Units**. Density, Depth and Temperature can be toggled independently between system international (SI “metric”) and U.S. customary units. For example, you can set the density to **lb/ft³** while the depth is set to **inches** and temperature is set for **celsius**.

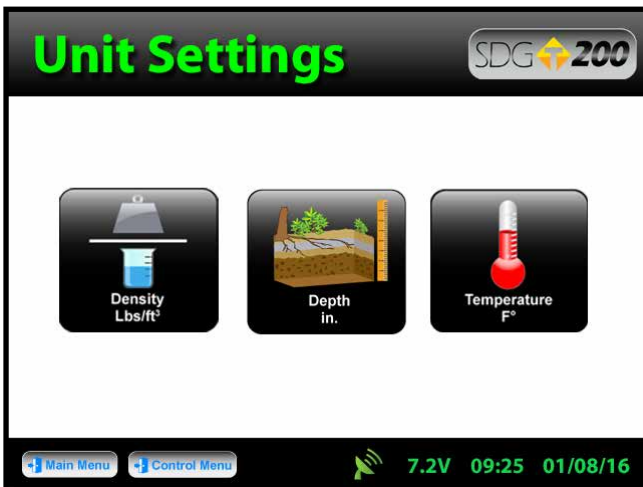

Material Details

From the **Control Menu**, press **Material** to enter the Material Details screen. The SDG 200 will store twenty detailed materials. The material highlighted in green on the left is displayed in detail on the right. To edit the details of this material, press **Edit Material**. **Note: Readings taken prior to accurately setting up the Material Details will result in incorrect density results.**

Material Details

SDG 200

Material ID: Coarse PL: 0.0
Description: Grainy LL: 0.0
Depth: 6.0 Cu: 4.4
Max Dry Density: 129.9 Cc: 0.94
Opt Moisture: 7.6

Wet Density Offset: 0.0
% Moisture Offset: 0.0
% Larger than 3": 0.0
% Larger than 3/4": 1.3
% Gravel: 6.4
% Sand: 87.6
% Fines: 6.0

Super Fine
Coarse
Fine

Edit Material
Upload Material

Main Menu Control Menu 7.2V 09:25 08/01/16

Edit Material

SDG 200

Material ID: Coarse
Description: Grainy
Depth: 6.0
Max Dry Density: 129.9
Opt Moisture: 7.6
Wet Density Offset: 0.0
% Moisture Offset: 0.0
% Larger Than 3": 0.0

Page 2

Main Menu Control Menu 7.2V 09:25 08/01/16

Edit Material

There are fifteen material properties for each material. Eight of these material properties are listed on page one of the edit material screen and the remaining seven are listed on page 2. Each can be edited individually by pressing its corresponding label which prompts a keyboard or alpha numeric keypad. For example, press **Material Name**, the keyboard will open allowing you to change the default name. Press **Clear** if you would like to start over with a new name. Press **Shift** to toggle from lowercase to uppercase letters. Once editing is complete, press the **Back** button located on page 2 of the edit material screen to verify your changes on the material details page.

The screenshot shows the 'Edit Material' interface. At the top left is a red 'Back' button with a left arrow. At the top right is a green 'Page 1' button with an up arrow. The main area contains eight input fields, each with a label and a value:

% Larger Than 3/4":	1.3
% Gravel:	6.4
% Sand:	87.6
% Fines:	6.0
PL:	0.0
LL:	0.0
Cu:	4.4
Cc:	0.94

At the bottom, there are two menu buttons: 'Main Menu' and 'Control Menu'. On the right, there is a signal strength icon, a battery level indicator '7.2V', and a clock '09:25' and date '08/01/16'.

The screenshot shows a virtual keyboard interface. At the top is a text input field containing the word 'Coarse'. Below the input field is a grid of buttons for numbers, letters, and symbols. The bottom row includes buttons for 'back space', 'space', 'shift', 'clear', and 'enter'.

Project Details


Keep track of your projects by entering detailed information into the project details screen. From the **Control Menu**, press **Project**. The green highlighted project is the **CURRENT PROJECT**. Readings taken will store in a text file with a .mnt extension using the **CURRENT PROJECT NAME**. You may revisit each project at any given time to continue taking readings. Data within each project will store in the order of which it was taken. To edit a project, press **Edit Project**. Press the button of the field you want to edit. When editing is complete press the **Back** button to save and return to the project details screen.



Soil Readings

From the **Control Menu**, press **Measure** to enter the **Soil Reading** screen. The name of the material to be tested and project are displayed for verification in the bottom right corner. The temperature of the soil is displayed on the left side of the screen, below that the GPS information is displayed. The cloverleaf measurement pattern is displayed for your convenience with the highlighted position being the current position to measure.


Position the gauge on the soil in position 1 as it appears on the screen and press **1**. **Do not touch the gauge while it is busy taking a measurement.** When reading 1 is complete, the gauge will prompt you to move to location 2. Move the gauge to position 2 and press **2** to continue. Repeat these steps for the remaining three measurements.

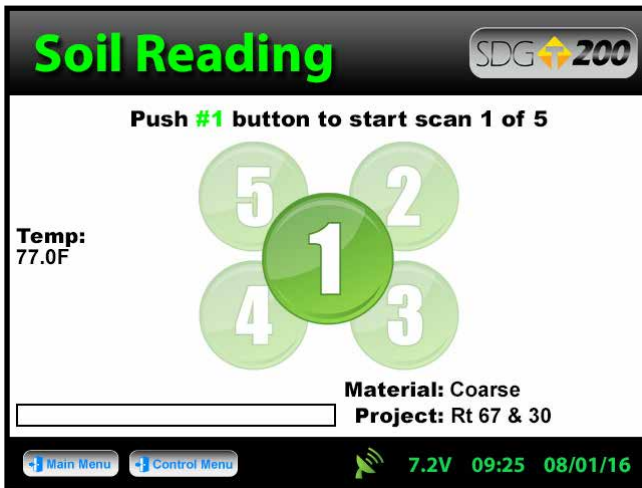

Soil Readings

After the fifth measurement has been taken, the in-place density and moisture content will be calculated and displayed on the screen. Here you can choose to **Accept** or **Reject** the recording of the averages into the data file. If you press **Accept**, you will enter the **Enter Location** screen allowing for a description of the location to be entered as well as the operator name.

Soil Reading



Temp: 77.0F

Compaction: 97%

% Moisture: 6.4

Wet Density: 134.1 lb/ft³

Dry Density: 126.0 lb/ft³

Material: Coarse

Project: Rt 67 & 30


Sats 5 42 47.19092 N 73 54.7338 W

Main Menu Control Menu 7.2V 09:25 08/01/16

Accept

Reject

Enter Location



Back

Description: First Measurement

Operator: Sean

Main Menu Control Menu 7.2V 09:25 08/01/16

Data Management

From the **Control Menu**, press **Data Management**. This is where project files will be saved, viewed, printed and downloaded.

Download Data - Use the up and down arrows to scroll, highlight the desired project and press **Download DAT & MNT**. Insert the USB flash drive into the USB port, press **Download**. The gauge will ask if you inserted the USB drive, once ready, press **Download**. When downloading is complete the gauge will display **READY**.

Viewing a Project File - Use the up and down arrows to scroll, highlight the desired project and press **View**. All of your tests saved to this project will be listed in the order they were taken. Only the most pertinent information will be shown in this view including: Test Number, Location, % Moisture, Wet Density, Dry Density, % Compaction. Press the **Back** button to exit the **Project View** screen.

Deleting a Project File - Use the up and down arrows to scroll, highlight the desired project and press **Delete**. You will be prompted with a warning asking if you are sure you wish to delete the file. Once confirmed and deleted, you will no longer be able to retrieve the measurement data.

Printing a Project File - Plug in your TransTech printer, use the up and down arrows to scroll, highlight the desired project and press **Print**.





Upload Material

The SDG 200 **MTL Generator** and **MTL File Tool** located on the support disk cd-rom (included in your kit) generates the text files needed to upload material data into the Material Details section of your gauge. Please see the SDG 200 Operator's Handbook for details on how to generate text files. Once your files are loaded onto a USB flash drive, insert the drive into the USB port on the back of the SDG 200. From the **Control Menu**, press **Material**, then press **Upload Material**.



Upload Material

Be sure to have your USB drive inserted into the USB port located on the back of the gauge then press **Upload**. The file name of the materials located on the USB drive will appear on the left and some details identifying that specific material will be displayed on the right. Use the up or down arrows to highlight the material you wish to upload. Once verified, press **Select** to upload the material information into the gauge. Press **Back** to view the uploaded material in detail.

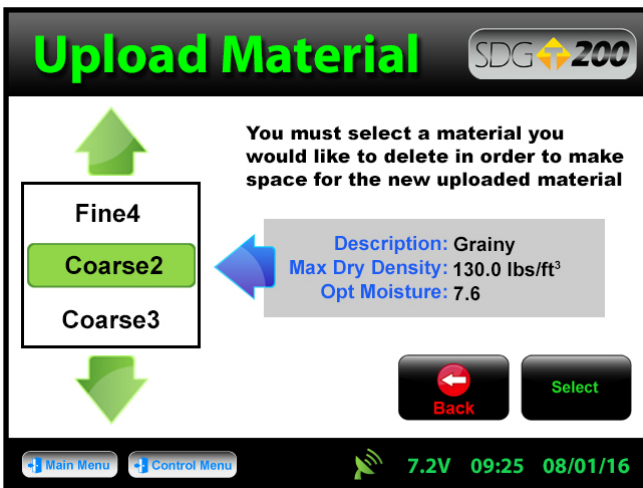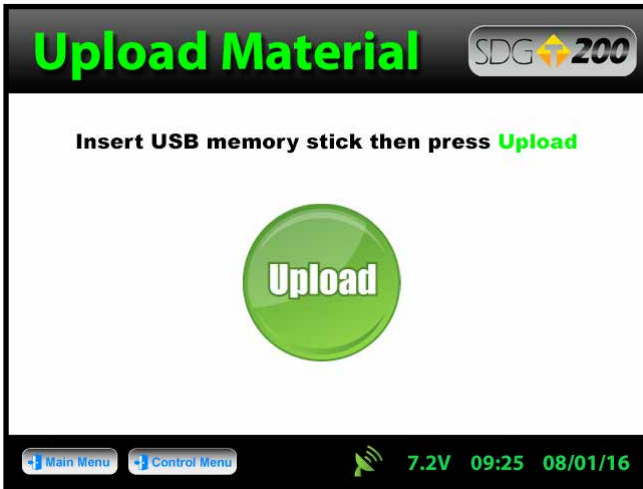

Upload Material

Note: Be sure that the units of the gauge are set for the same units as the material you are uploading. If the gauge was set in U.S. Customary units (ex: 150 lb/ft³) and you upload the material in SI units (2402.8 kg/m³) the gauge will notify you that the density is out of range. However, it will continue to load the material. If you switch to SI units AFTER the material has been loaded, the density would convert the 2402.8 as if it were in lb/ft³ and will result in 38,489.2 kg/m³.

Correct this by deleting the material, change the units of the gauge and reload the material or by simply editing the density in the material setup.

Material Details SDG 200

Material ID: Coarse2 **PL:** 0.0
Description: Grainy **LL:** 0.0
Depth: 6.0 **Cu:** 4.4
Max Dry Density: 130.0 **Cc:** 0.94
Opt Moisture: 7.6
Wet Density Offset: 0.0
% Moisture Offset: 0.0
% Larger than 3": 0.0
% Larger than 3/4": 1.3
% Gravel: 6.4
% Sand: 87.6
% Fines: 6.0

Super Fine
Coarse2
Fine

Edit Material
Upload Material

Main Menu Control Menu 7.2V 09:25 08/01/16

Replacement Parts

For a listing of replacement parts visit our website or contact your local distributor.

Warranty

TransTech Systems Product Warranty

The Company warrants to the Purchaser that the product delivered hereunder will be free from defects in material or workmanship and be the kind and quality designated or specified in the contract or purchase order. This warranty shall apply only to defects appearing within one (1) year from the date of shipment by the Company.

If the product delivered hereunder does not meet the above warranty and if the Purchaser promptly notifies the Company, the Company shall thereupon correct any defect, including nonconformance with the specifications, either (at the Company's option) by repairing any defective or damaged parts of the product, replacing the product, or by making available the necessary repaired or replacement parts.

The liability of the Company under this warranty, for any loss, whether the claim is based on contract or negligence, shall not in any case exceed the cost of correcting defects in the product as herein provided, and upon the expiration of the warranty period, all such liability shall terminate. The foregoing shall constitute the exclusive remedy of the Purchaser and the exclusive liability of the Company. The foregoing warranty is exclusive and in lieu of all other warranties, whether written, oral, implied or statutory.

No warranty of merchantability or of fitness for purpose shall apply. Unauthorized service shall void this warranty.

TransTech Systems Product Non-Warranty Return Policy

Non-warranty returns for TransTech Systems Inc. products must be made within ten (10) days from the original date of shipment, unless otherwise indicated. Returned products must be in the original packaging, unused and in undamaged condition. Proof of purchase is required. Upon receipt of the product TransTech will inspect the product to the above mentioned criteria.

Warranty

Unused products will be issued a credit to the Purchaser's account that was used to purchase the product. TransTech will not credit prepaid shipping cost. The original packing slip or invoice is required to be sent back with the product to be returned.

The Purchaser is responsible for shipping the product back to TransTech, carefully package the item(s) and include the packing slip and return manufacturing authorization number on the package. Prepay shipping is required – TransTech will not accept C.O.D.s.

Returns will be credited within 10 working days.


Proper Process of Warranty or Non-Warranty Shipments to TransTech Systems

For product returns (warranty or non-warranty), please follow the instructions below to assure prompt handling:

Call us for authorization (518-370-5558 or 800-724-6306), obtain a return manufacturing authorization number (RMA), and the return shipping address.

Indicate to our representative the reason for returning the product.

For Warranty Returns, Purchaser is responsible for shipping to TransTech's office. TransTech will pay ground shipping return to the Purchaser.



TransTech Systems, Inc.

**900 Albany Shaker Road, Suite 2
Latham, NY 12110**

Phone: 518-370-5558

Toll Free: 1-800-724-6306

Fax: 518-370-5538

Email: inquiries@transtechsys.com

Web: www.transtechsys.com

skype® Toll Free: [TransTech.Systems.Inc01](https://www.skype.com/join/TransTech.Systems.Inc01)

Follow us on



Rev-

06 /2023